

TRACEABLE® POCKET DIGITAL LIGHT METER INSTRUCTIONS

FEATURES

- Sensor used the exclusive photo diode & color correction filter
- High accuracy
- Light sensor probe allows user to measure light at an optimum position
- LCD display allows clear readout even in poor light conditions
- Pocket-sized, easy to carry & operate
- Compact, light weight and excellent operation
- Built-in low battery indicator

SPECIFICATIONS

Range: 0 to 1,999 foot-candles

Resolution: 0.1 to 1

Accuracy ±5% full scale + 4

LCD• 1/2-inch Display

Sensor diameter: 2 inches

Size: 2-3/4 x 5-1/4 x 1 inches

Weight: 6-1/2 ounces

OPERATION

1. Slide the "Off/On Switch" (3-2, Fig. 1) to the "On" position.
2. Select the maximum range on the "Range Switch" (3-3, Fig. 1).
3. Hold the "Light Sensor" (3-5, Fig. 1) by hand & face the measuring light opposite, then the Display (3-1, Fig. 1) will show light values directly.
4. Zero (offset) adjustment: For the normal operation, it is not necessary to make the Zero adjustment. However for the precise measurement, the following "Zero adjustment" procedures should be performed as:
 - a) Power on the meter
 - b) Select the measuring range: Range A (0 – 199.9 Fc, 3-3, Fig. 1)
 - c) Cover the Light Sensor (3-5, Fig. 1) completely.
 - d) Adjust the Zero Adjust VR (3-6, Fig. 1) until the display shows 0.

At range B (200 – 1,999 Fc) the unit shall display light values less than or equal to 200 Fc. If the measured light value falls below 200 Fc, select the "Range Switch" to lower the range (Range A) for a higher resolution reading.

BATTERY REPLACEMENT

1. When "LO BAT" appears on the LCD it is necessary to change the battery.
2. Slide the Battery Cover (3-4, fig. 1) away from the instrument and remove the battery.
3. Replace the 9V battery and replace the cover.
4. Make sure the battery cover is secured after changing the battery.

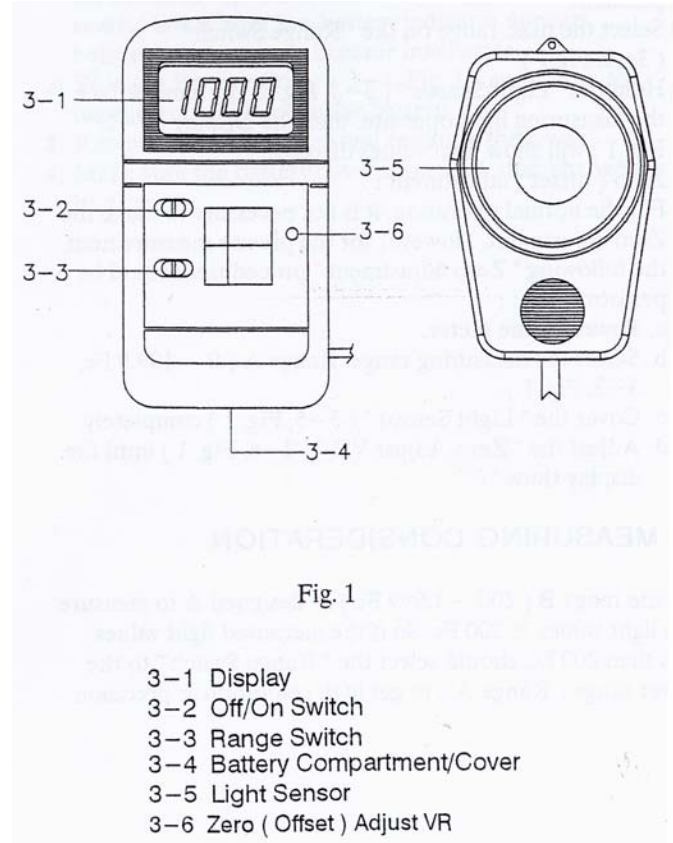


Fig. 1

- 3-1 Display
- 3-2 Off/On Switch
- 3-3 Range Switch
- 3-4 Battery Compartment/Cover
- 3-5 Light Sensor
- 3-6 Zero (Offset) Adjust VR

Warranty, Service, or Recalibration

For warranty, service, or recalibration, contact:

CONTROL COMPANY

4455 Rex Road
Friendswood, Texas 77546 USA
Ph. 281-482-1714
Fax 281-482-9448
E-mail sales@control3.com
www.control3.com

Control Company is ISO 9001 Quality-Certified by DNV and ISO 17025 accredited as a Calibration Laboratory by A2LA.

Control Company Cat. No. 3248

Traceable® is a registered trademark of Control Company

© 2010 Control Company 92-3248-00 Rev. 0 052410